

FIRST™ - Progesterone VGS 400 R

400 mg Progesterone Vaginal Suppository USP Compounding Kit

FOR PRESCRIPTION COMPOUNDING ONLY

DESCRIPTION



Each FIRST™ - Progesterone VGS 400 Compounding Kit is comprised of 12.0 grams of wettable progesterone USP powder and 57.0 grams of fatty acid base (hard fat NF).* FIRST™ - Progesterone VGS 400 Compounding Kit also contains the following components necessary to prepare 30 suppositories: 30-unit suppository mold w/caps, stirrer, suppository filling tool, guide plate, and 30-unit suppository mold protective cover w/suppository dispensing tool attached.

How Supplied and Compounding Directions







Size	30 Suppositories
NDC#	65628-064-01
Progesterone USP	12.0 g
Fatty Acid Base (Hard Fat NF)	57.0 g

TO THE PHARMACIST


Everything you need to make this R is included...

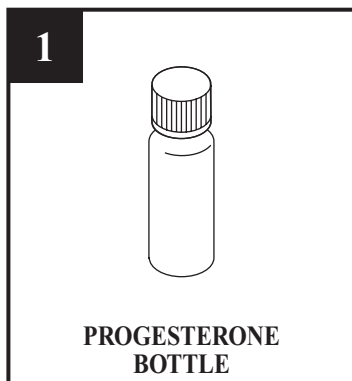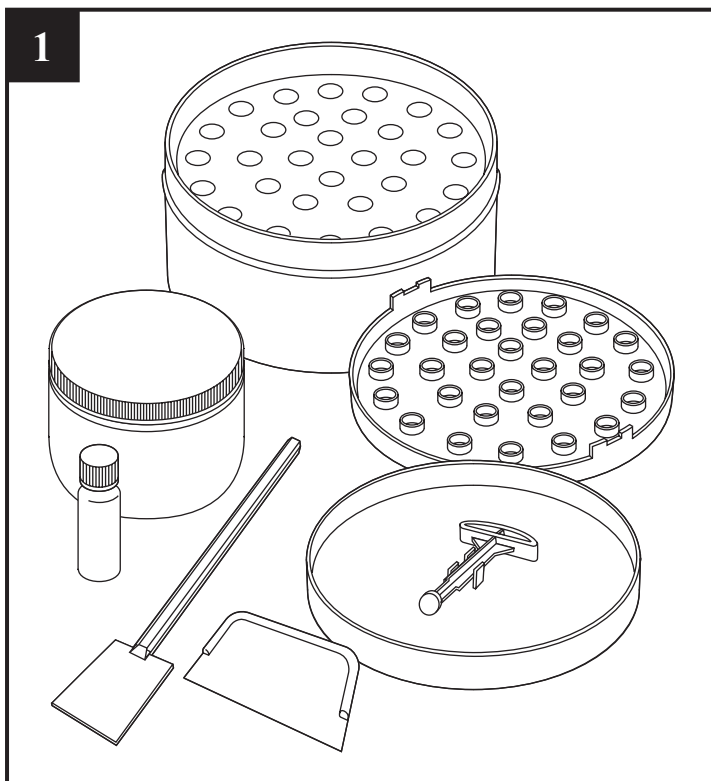


1. FIRST™ - Progesterone VGS 400 Compounding Kit contains pre-weighed progesterone powder and pre-weighed fatty acid base in sufficient quantity for the pharmacist to prepare 30 vaginal suppositories, each containing 400 mg of progesterone. **Important** - Prior to compounding and dispensing, read the instructions completely and make certain that all the components are present.

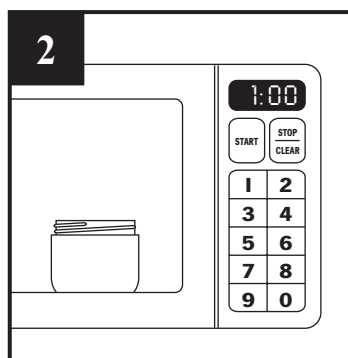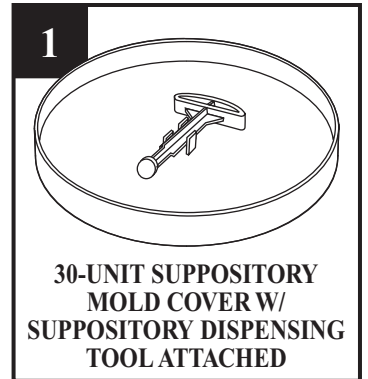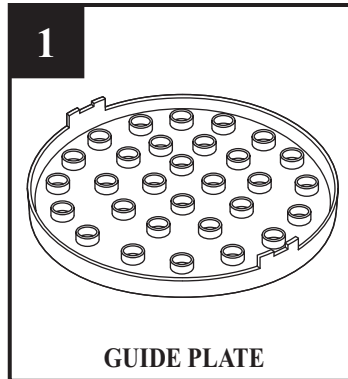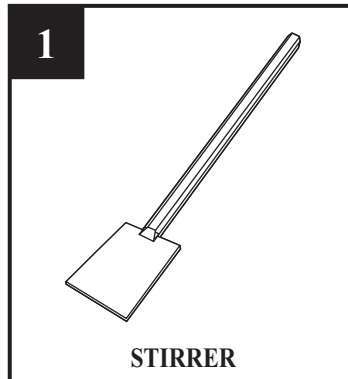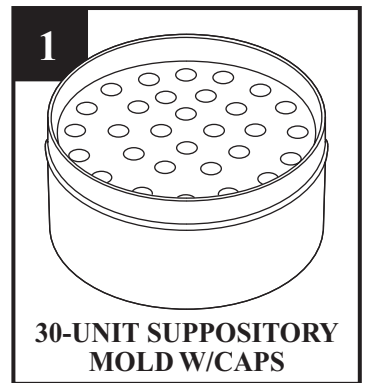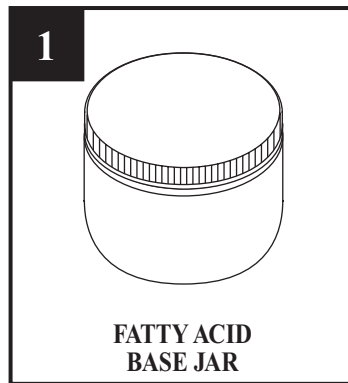


2. Remove the cap from jar containing fatty acid base and melt the base placing the jar in a standard microwave. **Melting times may vary depending on the type of microwave used.** It is recommended that you initially set the timer for 1 minute and check to see if the base has melted. If it has not, return the jar of base to the microwave for 15 second increments until the base is **completely** melted. Generally, the fatty acid base will completely melt between 1 and 3 minutes. **DO NOT OVERHEAT.**

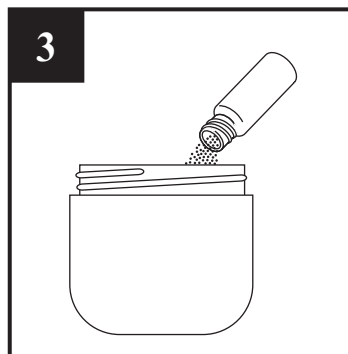


3. Tap the top and bottom of the bottle to loosen the progesterone powder and remove the cap. Empty the entire contents of the bottle into the jar containing the melted fatty acid base. It is recommended that you also tap the bottom and sides of the bottle while emptying. The appropriate quantity of progesterone powder has been packaged in the bottle to deliver enough progesterone to provide 400 mg for each suppository.

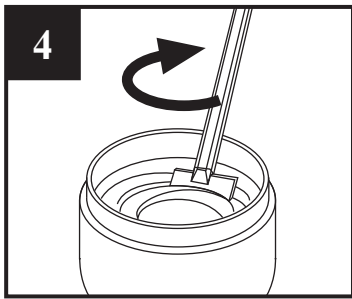


4. Using the stirrer provided, carefully stir the progesterone powder in the melted fatty acid base until an homogeneous suspension is apparent (60 to 90 seconds). **Be careful not to stir so vigorously as to spill the suspension outside the jar.**

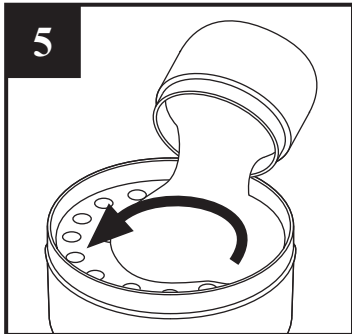


5. With an even flow, carefully pour the entire suspension from the jar onto the 30-unit suppository mold in a circular motion filling each of the 30 suppository cavities.

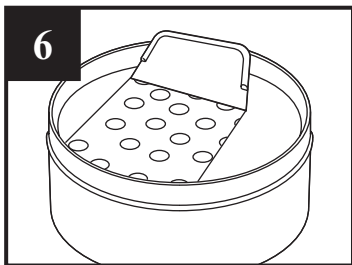


6. Using the suppository filling tool provided, spread the suspension evenly over the suppository cavities until all the cavities are completely filled.

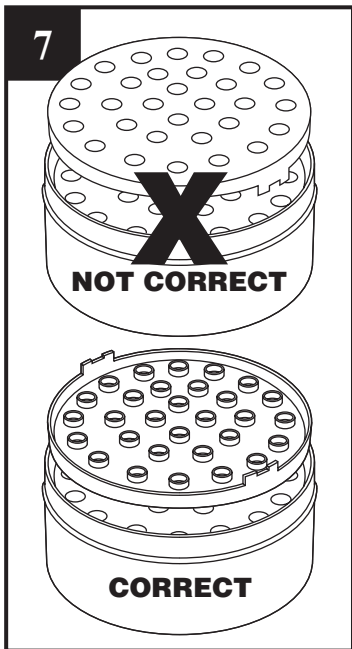

7. Place the provided guide plate onto the mold with the 30 raised guide holes facing upward. Make certain the notches on the guide plate align with notches on suppository mold. This will ensure that the 30 suppository cavities are aligned with the raised holes in the guide plate. Gently push the guide plate down to lock it in place. It is important that you fit the guide plate properly in order for your patient to dispense the suppositories easily.

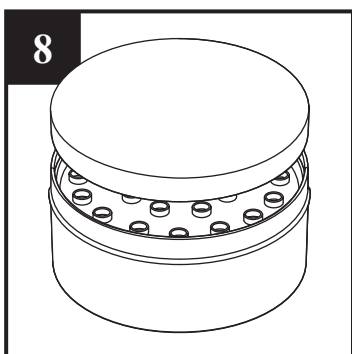

8. Place the provided cover with attached suppository dispensing tool onto the suppository mold. Store entire unit at refrigerated temperature for at least 15 minutes in order to allow the suppositories to solidify. Visually check the suppositories for solidification before dispensing the entire unit to your patient.

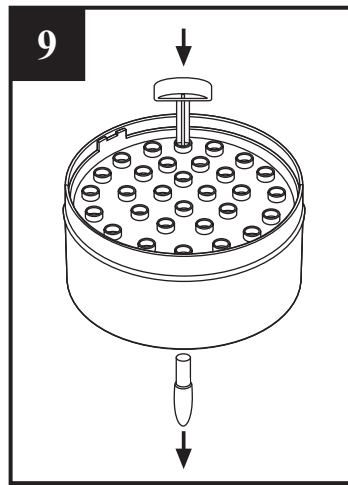

9. Make certain to instruct your patient how to dispense each suppository for daily use. Using the suppository dispensing tool attached to the mold cover, place the tip of the tool into the guide plate and with a firm force push the suppository through. Your patient should refrigerate the mold at least 1 hour for total solidification before dispensing the first suppository for use. **Important: Be sure to instruct your patient to remove the red suppository cap from the suppository before inserting each suppository.**

Prior to compounding, store FIRST™- Progesterone VGS 400 Compounding Kit at room temperature between 15°-30°C (59°-86°F) [see USP]. Also, store the compounded suppositories in the 30-unit suppository mold in the refrigerator (2°-8°C [36°-46°F]). FIRST™- Progesterone VGS 400 Compounding Kit components have a two-year expiration date.** The preparation of vaginal suppositories using FIRST™- Progesterone VGS 400 Compounding Kit complies with the requirements of USP, and as such, compounded suppositories made using FIRST™- Progesterone VGS 400 Compounding Kit can be used for up to ninety days after the day on which they were compounded.

When compounded and dispensed according to the instructions, average suppository weight has been found to be 2.3 grams and contain 90–110% of progesterone as labeled.**

The suppository mold and its accessories contained in this kit meet the requirements for USP Cytotoxicity Test, as well as Class VI Tests for plastic containers.**

Instruct patient as follows:

- For vaginal use only
- Do not take orally
- Do not insert in urinary opening or anus
- Avoid contact with eyes
- Keep out of reach of children
- Protect from light
- Keep container tightly closed
- Store suppositories in the mold, in the refrigerator
- Remove red caps from suppositories prior to use

* Certificate of analysis on file

** Data and documentation on file

R only

Issued: June 2006

U.S. Patents Pending

Distributed By:

CP CUTISPHARMA, INC.
SMART PRODUCTS FOR SMART PEOPLE™
 Beverly, MA 01915, USA www.cutispharma.com

